

Trade Term	FOB
Quantity	500,000PCS/
Lead Time	T/T
Production Cycle	3-7 days, 10-15 days
Payment Terms	T/T
Shipping Method	(DHL/UPS/FEDEX)
MOQ	100
Material	
Standards	CE, FCC, ROHS, REACH, UKCA

Notes:

ECG/EMG/EKG device is a medical device used for monitoring heart activity. It is important to ensure that the device is used correctly and that the data is accurate. The device is designed to be used by healthcare professionals and should not be used by laypeople. The device is subject to strict regulatory requirements and should be used in accordance with the manufacturer's instructions.

The device is available in various configurations and is suitable for use in a range of clinical settings. It is important to choose the right configuration for your application. The device is also available in different languages and can be used by people with different levels of proficiency.

The device is compatible with a range of operating systems and can be used on a variety of devices. It is important to ensure that the device is compatible with your system. The device is also available in different colors and can be used in a range of environments.


The device is designed to be easy to use and is suitable for use by people with different levels of proficiency. It is important to ensure that the device is used correctly and that the data is accurate. The device is also available in different languages and can be used by people with different levels of proficiency.

:







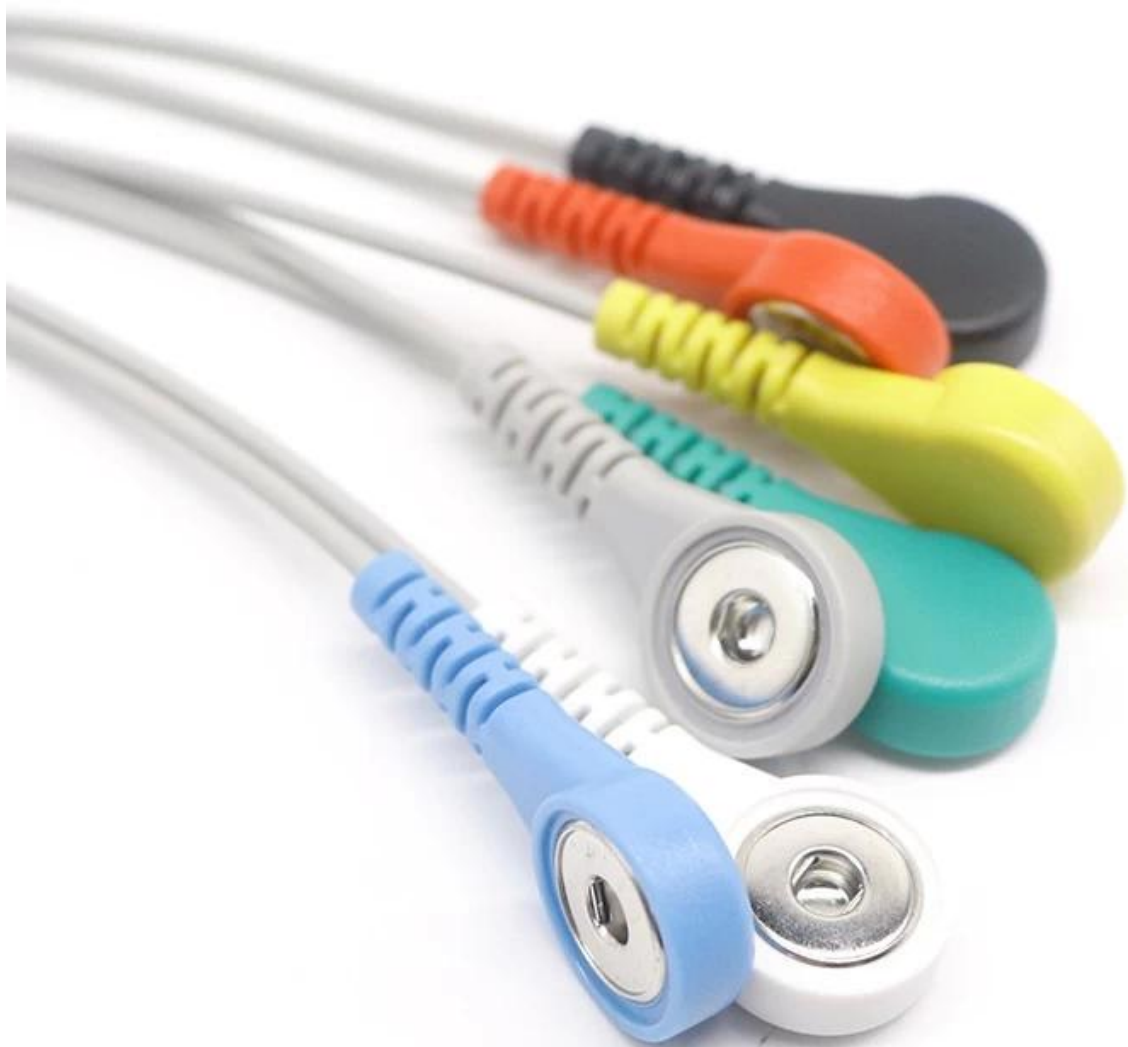



ZhongRen HeZong Certification (Shenzhen) Co., Ltd

Medical device management system mark of conformity

Certificate NO: 64622B80236ROS

We hereby certify that

Dongguan Goochain Technology Co., Ltd.

Unified Social Credit Code: 91441900MA4UTNP60C

Registered Address: Room 302, Building I, No. 8 Kangyang street, Shebei Village, Huangjiang Town, Dongguan City, Guangdong, China

Production / Business Address: Room 302, Building I, No. 8 Kangyang street, Shebei Village, Huangjiang Town, Dongguan City, Guangdong, China

Upon review, the organization's medical device management system meets the standards: :

YY/T0287-2017/ISO13485:2016

Certificate coverage:

Manufacturing and Sales for wires and cables that involves to Medical devices' s management activities.

Date of Issue: June 7, 2022

Date of Expiry: June 6, 2025

The First Surveillance	The Second Surveillance	The Third Surveillance
------------------------	-------------------------	------------------------

This certificate is used with the requirements of valid laws and regulations which the certification scope involved. The validity of the certificate should be confirmed and maintained through regular supervision and audit by ZhongRen HeZong Certification Co., Ltd. Please conduct supervision and audit according to the annual audit time. If you fail to pass the audit within the time limit, the certificate will be invalid.

Check the CNCA Website: www.cnca.gov.cn
Or website of company: www.zrhz-cert.com



Address: R606, Jiayu Building, Hongxing Community, Songgang Street, Bao'an District, Shenzhen.
Tel: 0755-23305084 Website: www.zrhz-cert.com

